



Proudly Owned and Operated in the USA

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

|                            |                                                                                  |
|----------------------------|----------------------------------------------------------------------------------|
| <b>Product</b>             | KLOW 10/50mg                                                                     |
| <b>Net Peptide Content</b> | GHK-Cu- 46.83 mg<br>KPV- 9.48 mg<br>BPC-157- 8.74 mg<br>Thymosin Beta-4- 8.33 mg |
| <b>Identity</b>            | GHK-Cu/KPV/BPC-157/<br>Thymosin Beta-4                                           |

## Certificate of Analysis



|                         |                       |
|-------------------------|-----------------------|
| <b>Accession Number</b> | 2511260090            |
| <b>Client</b>           | Felix Chemical Supply |
| <b>Search Code</b>      | Feli2511260090        |

|                       |            |
|-----------------------|------------|
| <b>Received Date:</b> | 11/26/2025 |
| <b>Reported Date:</b> | 11/30/2025 |

|                   |                         |
|-------------------|-------------------------|
| <b>Lot</b>        | 112425-KLO-C            |
| <b>Purity</b>     | 99.87%                  |
| <b>Appearance</b> | Blue Lyophilized Powder |

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

|                                           |               |
|-------------------------------------------|---------------|
| <b>Mass Identification</b>                | <b>Result</b> |
| <b>GHK-Cu/KPV/BPC-157/Thymosin Beta-4</b> | <b>99.87%</b> |

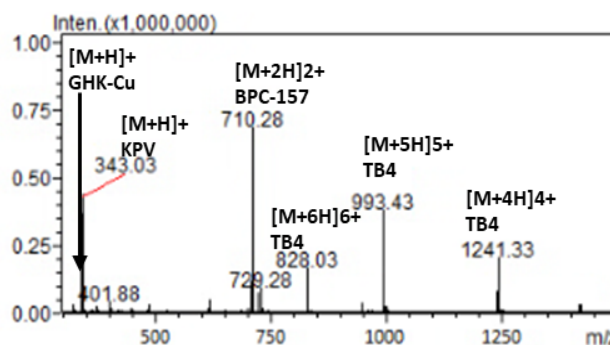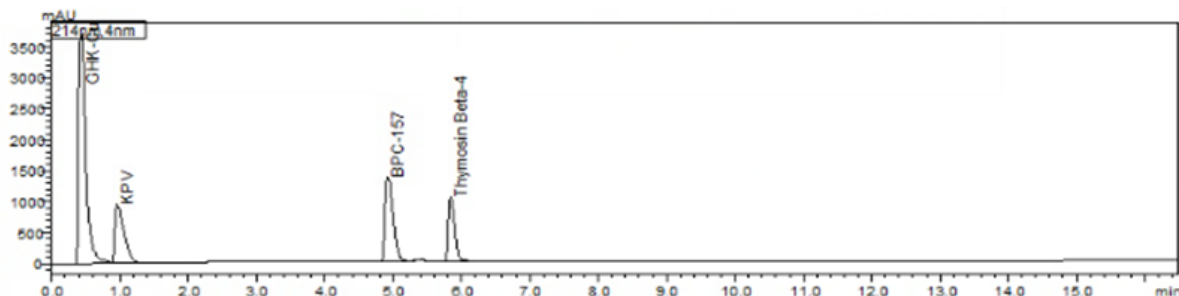

*Stephen Schmidt*

**COA: 2511260090**

Stephen Schmidt  
Principal Chemist

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Contact at: [Admin@FreedomDiagnostics.net](mailto:Admin@FreedomDiagnostics.net)



Proudly Owned and Operated in the USA

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

|         |              |
|---------|--------------|
| Product | KLOW 10/50mg |
|---------|--------------|

## Certificate of Analysis

|                  |                       |
|------------------|-----------------------|
| Accession Number | 2511260091            |
| Client           | Felix Chemical Supply |
| Search Code      | Feli2511260091        |

|                |            |
|----------------|------------|
| Received Date: | 11/26/2025 |
| Reported Date: | 11/30/2025 |

|     |              |
|-----|--------------|
| Lot | 112425-KLO-C |
|-----|--------------|

All analyses are conducted for research purposes and performed in duplicate in accordance with USP <85> guidelines

| Endotoxin Threshold |                   | Result |
|---------------------|-------------------|--------|
| Replicate 1         | $\leq 0.05$ EU/mL | Pass   |
| Replicate 2         | $\leq 0.05$ EU/mL | Pass   |



*Stephen Schmidt*

Stephen Schmidt  
Principal Chemist

**COA: 2511260091**

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: [FreedomDiagnosticsTesting.com](https://freedomdiagnostics.com)

Contact at: [Admin@FreedomDiagnostics.net](mailto:Admin@FreedomDiagnostics.net)